


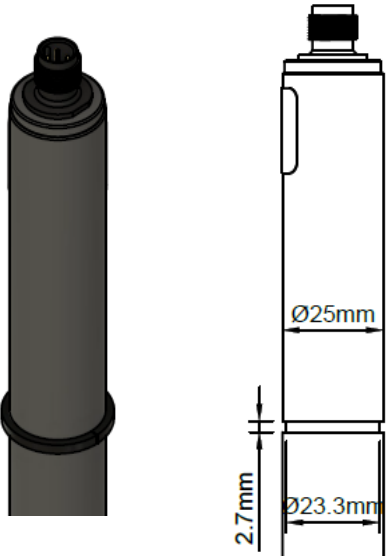
	<h1>TARAbase CL4.2</h1>				
indicator	Free chlorine, pH-dependent				
Application	Swimming pool water, drinking water, service water, process water The water must not contain any surfactants (tensides)! pH-value must be constant.				
Chlorination agents	inorganic chlorine compounds: NaOCl (=sodium hypochlorite), Ca(OCl) ₂ , chlorine gas, chlorine electrolysis with membrane cell (unsuitable: chlorine electrolysis without membrane cell)				
Measuring system	Membrane covered, amperometric 2-electrode system with electronic inside				
Electronic	<p>Analog version:</p> <ul style="list-style-type: none"> - voltage output - not galvanically isolated electronics - analog internal data processing - output signal: analog (analog-out/analog) <p>Digital version:</p> <ul style="list-style-type: none"> - electronic is completely galvanically isolated - digital internal data processing - output signal: analog (analog-out/digital) or digital (digital-out/digital) <p>mA-version:</p> <ul style="list-style-type: none"> - current output analog - not galvanically isolated electronics - output signal: analog (analog-out/analog) 				
Information about the measuring range	<p>The actual slope of a sensor can vary production-related between 65% and 150% of the nominal slope</p> <p>Note: With a slope > 100% the measuring range is reduced accordingly. (Ex.: 150% slope → 67% of the specified measuring range)</p>				
Accuracy after calibration at repeatability conditions (25°C, pH 7.2 in drinking water) of the upper full scale	<p>– Measuring range 2 mg/l:</p> <table style="margin-left: 40px;"> <tr> <td>at 0.4 mg/l</td> <td><1%</td> </tr> <tr> <td>at 1.6 mg/l</td> <td><1%</td> </tr> </table>	at 0.4 mg/l	<1%	at 1.6 mg/l	<1%
at 0.4 mg/l	<1%				
at 1.6 mg/l	<1%				
Slope drift At repeatability conditions (25 °C, pH 7,2 in drinking water)	approx. <-1% per month				
Working temperature	Measuring water temperature: 0 ... +45 °C (no ice crystals in the measuring water)				
	Ambient temperature: 0 ... +55 °C				
Temperature compensation	Automatically, by an integrated temperature sensor Sudden temperature changes must be avoided				


	<h1>TARAbase CL4.2</h1>	
Max. allowed working pressure	Operation without retaining ring: – 0.5 bar – no pressure impulses and/or vibrations Operation with retaining ring in TARAflow FLC: – 1 bar, – no pressure impulses and/or vibrations (see option 1)	
Flow rate (Incoming flow velocity)	approx. 15-30/h (33 – 66 cm/s) in TARAflow FLC, small flow rate dependence is given (see diagram “Slope of TARAbase CL4 versus flowrate”, p. 8)	
pH-range	pH 6 – pH 8, pay attention to the dissociation equilibrium HOCL (see diagram “Slope of TARAbase CL4 versus pH, p. 8)	
Run-in time	First start-up approx. 1 h	
Response time	T_{90} : approx. 30 sec.	
Zero point adjustment	Not necessary	
calibration	At the device, by analytical determination DPD-1-Method	
Interferences	ClO_2 : factor 9 O_3 Electrolytically generated chlorine with a cell without membrane can produce trouble	
Absence of the disinfectant	Max. 24 h	
Connection	mV version: 5-pole M12, plug-on flange Modbus version: 5-pole M12, plug-on flange 4-20 mA version: 2-pole terminal or 5-pole M12, plug-on flange	
max. length of sensor cable (depending on internal signal processing)	analog	< 30 m
	digital	> 30 m are permissible Maximum cable length depends on application
Protection type	5-pole M12 plug-on flange: IP68 2-pole terminal with mA-hood: IP65	
material	Semipermeable membrane, PVC-U, ABS	
Size	diameter: approx. 25 mm Length: mV version approx. 190 mm (analog signal processing) approx.. 205 mm (digital signal processing) Modbus version approx. 205 mm 4-20 mA version approx. 220 mm (2-pole-terminal) approx. 190 mm (5-pole-M12)	

	<h1>TARAbase CL4.2</h1>	
<p>Transport</p>	<p>+5 ... +50 °C (sensor, electrolyte, membrane cap)</p>	
<p>storage</p>	<p>Sensor: dry and without electrolyte no limit at +5 ... +40 °C</p>	<p>Electrolyte: in original bottle protected from sunlight at +5 ... +35 °C min. 1 year or until specified EXP-Date</p>
	<p>Membrane cap: in original packing no limit at +5 ... +40 °C (used membrane caps can not be stored)</p>	
	<p>Regularly control of the measuring signal, min. once a week The following specifications depend on the water quality: Change of the membrane cap: once a year Change of the electrolyte: every 3 - 6 months</p>	
	<p>EMC tested RoHS compliant</p>	

<p>Option 1: Retaining ring</p>	<ul style="list-style-type: none"> - When operating with pressures >0.5 bar in TARAflow FLC - Dimensions retaining ring 29 x 23.4 x 2.5 mm, slitted, PETP - Different positions for groove selectable (on request) 	
--	--	--

Technical Data
1. CL4.2 (analog output, analog internal signal processing)


A potential-free electrical connection is necessary as the sensor electronic is not equipped with a galvanical isolation.

	Measuring range in ppm	resolution in ppm	Output Output resistance	Nominal slope (at pH 7.2) in mV/ppm	Voltage supply	Connection
CL4.2N-M12	0.05...20.00	0.01	0...-2000 mV 1 kΩ	-100	±5 - ±15 VDC 10 mA	5-pole M12 plug-on flange Function of wires: PIN1: measuring signal PIN2: +U PIN3: -U PIN4: signal GND PIN5: n. c.
CL4.2H-M12	0.005...2.000	0.001		-1000		
CL4.2DW-M12	0.005...5.000	0.001		-300		
CL4.2L-M12	0.5...200.0	0.1		-10		
CL4.2Hup-M12	0.005...2.000	0.01	0...+2000 mV 1 kΩ	+1000	10 - 30 VDC 10 mA	5-pole M12 plug-on flange Function of wires: PIN1: measuring signal PIN2: +U PIN3: power GND PIN4: signal GND PIN5: n. c.
CL4.2Up-M12	0.05...20.00	0.01		+100		

(Subject to technical changes!)

2. CL4.2 (analog output, digital internal signal processing) analog-out / digital


- The power supply is galvanically isolated inside of the sensor.
- The output signal is galvanically isolated too, that means potential-free.

	Measuring range in ppm	resolution in ppm	Output Output resistance	Nominal slope (at pH 7.2) in mV/ppm	Power supply	Connection
CL4.2H-An-M12	0.005...2.000	0.001	analog 0...-2 V (max. -2.5 V) 1 kΩ	-1000	9-30 VDC approx. 20-56 mA	5-pole M12 plug-on flange Function of wires: PIN1: measuring signal PIN2: +U PIN3: power GND PIN4: signal GND PIN5: n. c.
CL4.2N-An-M12	0.05...20.00	0.01		-100		
CL4.2L-An-M12	0.5...200.0	0.1		-10		
CL4.2H-Ap-M12	0.005...2.000	0.001	analog 0...+2 V (max. +2.5 V) 1 kΩ	+1000		
CL4.2N-Ap-M12	0.05...20.00	0.01		+100		
CL4.2L-Ap-M12	0.5...200.0	0.1		+10		

(Subject to technical changes!)

3. CL4.2 (digital output, digital internal signal processing)

- The power supply is galvanically isolated inside of the sensor.
- The output signal is galvanically isolated too, that means potential-free.


	Measuring range in ppm	resolution in ppm	Output Output resistance	Power supply	Connection
CL4.2H-M0c	0.005... 2.000	0.001	Modbus RTU There are no terminating resistors in the sensor.	9-30 VDC approx. 20-56 mA	5-pole M12 plug-on flange Function of wires: PIN1: reserved PIN2: +U PIN3: power GND PIN4: RS485B PIN5: RS485A
CL4.2N-M0c	0.05... 20.00	0.01			
CL4.2L-M0c	0.5...200.0	0.1			

(Subject to technical changes!)

4. CL4.2 4-20 mA (analog output, analog internal signal processing)


A potential-free electrical connection is necessary as the sensor electronic is not equipped with a galvanical isolation.

4.1 Electrical connection: 2 pole terminal clamp

	Measuring range	Resolution	Output Output resistance	Nominal slope (at pH 7.2)	Voltage supply	Connection
	in ppm	in ppm		in mA/ppm		
CL4.2MA0.5	0.005...0.500	0.001	4...20 mA uncalibrated	32.0	12...30 VDC R _L 50Ω...R _L 900Ω	2-pole terminal (2 x 1 mm ²) Recommended: Round cable ∅ 4 mm 2 x 0.34 mm ²
CL4.2MA2	0.005...2.000	0.001		8.0		
CL4.2MA5	0.05...5.00	0.01		3.2		
CL4.2MA10	0.05...10.00	0.01		1.6		
CL4.2MA20	0.05...20.00	0.01		0.8		
CL4.2MA-100	0.5...100.0	0.1		0.16		
CL4.2MA-200	0.5...200.0	0.1		0.8		

(Subject to technical changes!)

4.2 Electrical connection: 5 pole M12 plug-on flange

	Measuring range	resolution	Output Output resistance	Nominal slope (at pH 7.2)	Voltage supply	Connection
	in ppm	in ppm		in mA/ppm		
CL4.2MA0.5-M12	0.005...0.500	0.001	4...20 mA uncalibrated	32.0	12...30 VDC R _L 50Ω...R _L 900Ω	5-pole M12 plug-on flange Function of wires: PIN1: n. c. PIN2: +U PIN3: -U PIN4: n. c. PIN5: n. c.
CL4.2MA2-M12	0.005...2.000	0.001		8.0		
CL4.2MA5-M12	0.05...5.00	0.01		3.2		
CL4.2MA10-M12	0.05...10.00	0.01		1.6		
CL4.2MA20-M12	0.05...20.00	0.01		0.8		
CL4.2MA-100-M12	0.5...100.0	0.1		0.16		
CL4.2MA-200-M12	0.5...200.0	0.1		0.8		

(Subject to technical changes!)


Spare Parts

Type	Membrane cap	Electrolyte	Emery	O-ring
For all CL4.2	M20.2 Art. no. 11011.1	ECL1, 100 ml Art. no. 11001	S1 Art. no. 11908	14 x 1.8 NBR Art. No. 11806

(Subject to technical changes!)

Slope of TARAbase CL4 versus pH


Temperature: 25°C / Flow rate: 30 l/h

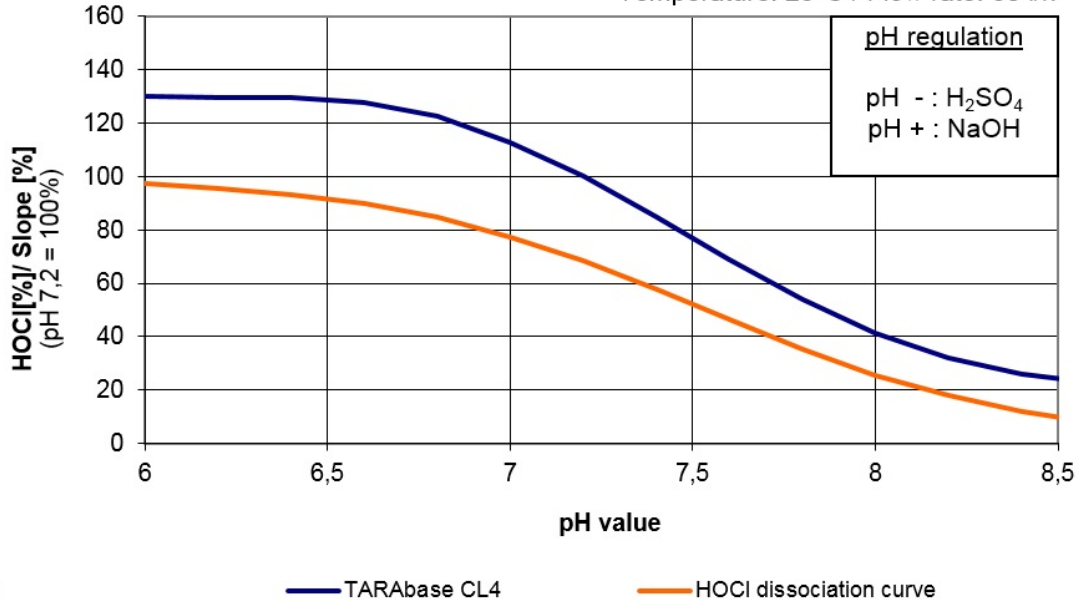

CL-Dringmann

Slope of TARAbase CL4 versus Flow rate

Temperature: 25°C / pH value: 7,2

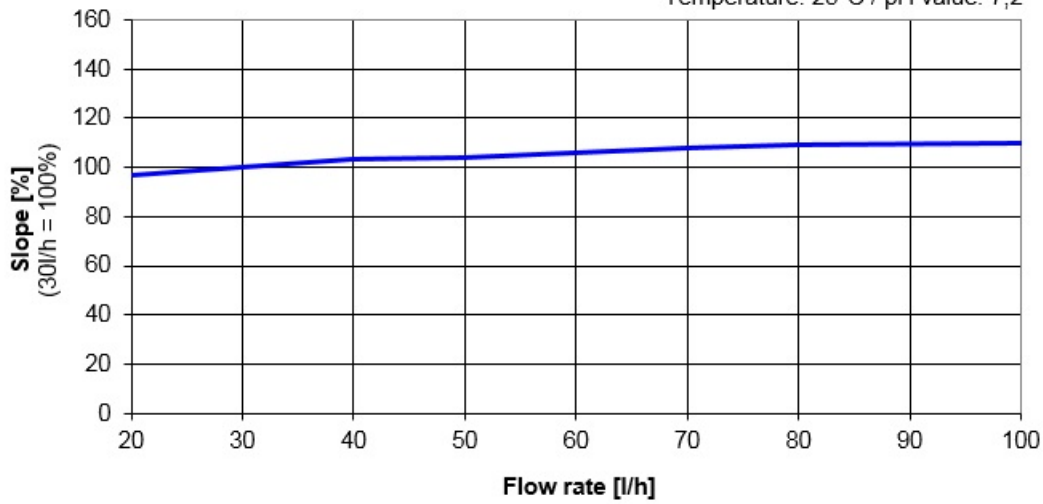

CL-Dringmann

This values are only valid for the probe housing FLC1 / FLC3