


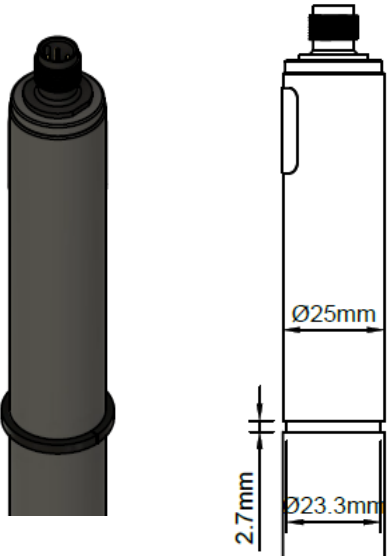

	<h1>TARAbase CL4.2</h1>								
indicator	Free chlorine, pH-dependent								
Application	Swimming pool water, drinking water, service water, process water The water must not contain any surfactants (tensides)! pH-value must be constant.								
Chlorination agents	inorganic chlorine compounds: NaOCl (=sodium hypochlorite), Ca(OCl) ₂ , chlorine gas, chlorine electrolysis with membrane cell (unsuitable: chlorine electrolysis without membrane cell)								
Measuring system	Membrane covered, amperometric 2-electrode system with electronic inside								
Electronic	Analog version: <ul style="list-style-type: none"> - voltage output - not galvanically isolated electronics - analog internal data processing Digital version: <ul style="list-style-type: none"> - electronic is completely galvanically isolated - digital internal data processing - output signal: analog (analog-out/digital) or digital (digital-out/digital) mA-version: <ul style="list-style-type: none"> - current output analog - not galvanically isolated electronics - output signal: analog (analog-out/analog) 								
Information about the measuring range	The actual slope of a sensor can vary production-related between 65% and 150% of the nominal slope Note: With a slope > 100% the measuring range is reduced accordingly. (Ex.: 150% slope → 67% of the specified measuring range)								
Accuracy after calibration at repeatability conditions (25°C, pH 7.2 in drinking water) of the upper full scale	<table border="0" style="width: 100%;"> <tr> <td style="width: 40%;">– Measuring range 2 mg/l:</td> <td style="width: 20%;">at 0.4 mg/l</td> <td style="width: 20%; text-align: right;"><1%</td> <td style="width: 20%;"></td> </tr> <tr> <td></td> <td>at 1.6 mg/l</td> <td style="text-align: right;"><1%</td> <td></td> </tr> </table>	– Measuring range 2 mg/l:	at 0.4 mg/l	<1%			at 1.6 mg/l	<1%	
– Measuring range 2 mg/l:	at 0.4 mg/l	<1%							
	at 1.6 mg/l	<1%							
Slope drift At repeatability conditions (25 °C, pH 7,2 in drinking water)	approx. <-1% per month								
Working temperature	Measuring water temperature: 0 ... +45 °C (no ice crystals in the measuring water)								
	Ambient temperature: 0 ... +55 °C								
Temperature compensation	Automatically, by an integrated temperature sensor Sudden temperature changes must be avoided								

	<h1>TARAbase CL4.2</h1>																			
<p>Max. allowed working pressure</p>	<p>Operation without retaining ring:</p> <ul style="list-style-type: none"> - 0.5 bar - no pressure impulses and/or vibrations <p>Operation with retaining ring in TARAflow FLC:</p> <ul style="list-style-type: none"> - 1 bar, - no pressure impulses and/or vibrations (see option 1) 																			
<p>Flow rate (Incoming flow velocity)</p>	<p>approx. 15-30/h (15 – 30 cm/s) in TARAflow FLC, small flow rate dependence is given (see diagram “Slope of TARAbase CL4 versus flowrate”)</p>																			
<p>pH-range</p>	<p>pH 6 – pH 8, pay attention to the dissociation equilibrium HOCl (see diagram “Slope of TARAbase CL4 versus pH”)</p>																			
<p>Run-in time</p>	<p>First start-up approx. 1 h</p>																			
<p>Response time</p>	<p>T₉₀: approx. 30 sec.</p>																			
<p>Zero point adjustment</p>	<p>Not necessary</p>																			
<p>calibration</p>	<p>At the device, by analytical determination DPD-1-Method</p>																			
<p>Interferences</p>	<p>ClO₂: factor 9 O₃ Electrolytically generated chlorine with a cell without membrane can produce trouble</p>																			
<p>Absence of the disinfectant</p>	<p>Max. 24 h</p>																			
<p>Connection</p>	<table style="width: 100%; border: none;"> <tr> <td style="width: 33%; border: none;">mV version:</td> <td style="border: none;">5-pole M12, plug-on flange</td> </tr> <tr> <td style="border: none;">Modbus version:</td> <td style="border: none;">5-pole M12, plug-on flange</td> </tr> <tr> <td style="border: none;">4-20 mA version:</td> <td style="border: none;">2-pole terminal</td> </tr> <tr> <td style="border: none;"></td> <td style="border: none;">or</td> </tr> <tr> <td style="border: none;"></td> <td style="border: none;">5-pole M12, plug-on flange</td> </tr> </table>		mV version:	5-pole M12, plug-on flange	Modbus version:	5-pole M12, plug-on flange	4-20 mA version:	2-pole terminal		or		5-pole M12, plug-on flange								
mV version:	5-pole M12, plug-on flange																			
Modbus version:	5-pole M12, plug-on flange																			
4-20 mA version:	2-pole terminal																			
	or																			
	5-pole M12, plug-on flange																			
<p>max. length of sensor cable (depending on internal signal processing)</p>	<p>analog</p>	<p>< 30 m</p>																		
	<p>digital</p>	<p>> 30 m are permissible Maximum cable length depends on application</p>																		
<p>Protection type</p>	<table style="width: 100%; border: none;"> <tr> <td style="width: 60%; border: none;">5-pole M12 plug-on flange:</td> <td style="border: none;">IP68</td> </tr> <tr> <td style="border: none;">2-pole terminal with mA-hood:</td> <td style="border: none;">IP65</td> </tr> </table>		5-pole M12 plug-on flange:	IP68	2-pole terminal with mA-hood:	IP65														
5-pole M12 plug-on flange:	IP68																			
2-pole terminal with mA-hood:	IP65																			
<p>material</p>	<p>Semipermeable membrane, PVC-U, ABS</p>																			
<p>Size</p>	<table style="width: 100%; border: none;"> <tr> <td style="width: 33%; border: none;">diameter:</td> <td colspan="2" style="border: none;">approx. 25 mm</td> </tr> <tr> <td style="border: none;">Length: mV version</td> <td colspan="2" style="border: none;">approx. 190 mm (analog signal processing)</td> </tr> <tr> <td style="border: none;"></td> <td colspan="2" style="border: none;">approx. 205 mm (digital signal processing)</td> </tr> <tr> <td style="border: none;">Modbus version</td> <td colspan="2" style="border: none;">approx. 205 mm</td> </tr> <tr> <td style="border: none;">4-20 mA version</td> <td colspan="2" style="border: none;">approx. 220 mm (2-pole-terminal)</td> </tr> <tr> <td style="border: none;"></td> <td colspan="2" style="border: none;">approx. 190 mm (5-pole-M12)</td> </tr> </table>		diameter:	approx. 25 mm		Length: mV version	approx. 190 mm (analog signal processing)			approx. 205 mm (digital signal processing)		Modbus version	approx. 205 mm		4-20 mA version	approx. 220 mm (2-pole-terminal)			approx. 190 mm (5-pole-M12)	
diameter:	approx. 25 mm																			
Length: mV version	approx. 190 mm (analog signal processing)																			
	approx. 205 mm (digital signal processing)																			
Modbus version	approx. 205 mm																			
4-20 mA version	approx. 220 mm (2-pole-terminal)																			
	approx. 190 mm (5-pole-M12)																			

	<h1>TARAbase CL4.2</h1>	
<p>Transport</p>	<p>+5 ... +50 °C (sensor, electrolyte, membrane cap)</p>	
<p>storage</p>	<p>Sensor: dry and without electrolyte no limit at +5 ... +40 °C</p>	<p>Electrolyte: in original bottle protected from sunlight at +5 ... +35 °C min. 1 year or until specified EXP-Date</p>
	<p>Membrane cap: in original packing no limit at +5 ... +40 °C (used membrane caps can not be stored)</p>	
	<p>Regularly control of the measuring signal, min. once a week The following specifications depend on the water quality: Change of the membrane cap: once a year Change of the electrolyte: every 3 - 6 months</p>	
	<p>EMC tested RoHS compliant</p>	

<p>Option 1: Retaining ring</p>	<ul style="list-style-type: none"> - When operating with pressures >0.5 bar in TARAflow FLC - Dimensions retaining ring 29 x 23.4 x 2.5 mm, slitted, PETP - Different positions for groove selectable (on request) 	
--	--	--


Technical Data
1. CL4.2 (analog output, analog internal signal processing)

	Measuring range in ppm	Resolution in ppm	Output Output resistance	Nominal slope (at pH 7.2) in mV/ppm	Voltage supply	Galvanic isolation required in the measuring device/controller *	Connection
CL4.2N-M12	0.05...20.00	0.01	0...-2000 mV 1 kΩ	-100	±5 - ±15 VDC 10 mA	yes	5-pole M12 plug-on flange Function of wires: PIN1: measuring signal PIN2: +U PIN3: -U PIN4: signal GND PIN5: n. c.
CL4.2H-M12	0.005...2.000	0.001		-1000			
CL4.2DW-M12	0.005...5.000	0.001		-300			
CL4.2L-M12	0.5...200.0	0.1		-10			
CL4.2HU _p -M12	0.005...2.000	0.01	0...+2000 mV 1 kΩ	+1000	10 - 30 VDC 10 mA		5-pole M12 plug-on flange Function of wires: PIN1: measuring signal PIN2: +U PIN3: power GND PIN4: signal GND PIN5: n. c.
CL4.2U _p -M12	0.05...20.00	0.01		+100			

* for further information see brochure 'Technical information // galvanic isolation' (in the download area of our website www.reiss-gmbh.com)

(Subject to technical changes!)


2. CL4.2 (analog output, digital internal signal processing)
analog-out / digital

	Measuring range in ppm	Resolution in ppm	Output Output resistance	Nominal slope (at pH 7.2) in mV/ppm	Power supply	Galvanic isolation required in the measuring device/controller *	Connection
CL4.2H-An-M12	0.005...2.000	0.001	analog 0...-2 V (max. -2.5 V) 1 kΩ	-1000	9-30 VDC approx. 7-30 mA	no	5-pole M12 plug-on flange Function of wires: PIN1: measuring signal PIN2: +U PIN3: power GND PIN4: signal GND PIN5: n. c.
CL4.2N-An-M12	0.05...20.00	0.01		-100			
CL4.2L-An-M12	0.5...200.0	0.1		-10			
CL4.2H-Ap-M12	0.005...2.000	0.001	analog 0...+2 V (max. +2.5 V) 1 kΩ	+1000			
CL4.2N-Ap-M12	0.05...20.00	0.01		+100			
CL4.2L-Ap-M12	0.5...200.0	0.1		+10			

* for further information see brochure 'Technical information // galvanic isolation' (in the download area of our website www.reiss-gmbh.com)

(Subject to technical changes!)

3. CL4.2 (digital output, digital internal signal processing)


	Measuring range in ppm	Resolution in ppm	Output Output resistance	Power supply	Galvanic isolation required in the measuring device/controller *	Connection
CL4.2H-M0c	0.005... 2.000	0.001	Modbus RTU There are no terminating resistors in the sensor.	9-30 VDC approx. 7-30 mA	no	5-pole M12 plug-on flange Function of wires: PIN1: reserved PIN2: +U PIN3: power GND PIN4: RS485B PIN5: RS485A
CL4.2N-M0c	0.05... 20.00	0.01				
CL4.2L-M0c	0.5...200.0	0.1				

* for further information see brochure 'Technical information // galvanic isolation' (in the download area of our website www.reiss-gmbh.com)

(Subject to technical changes!)

4. CL4.2 4-20 mA (analog output, analog internal signal processing)


4.1 Electrical connection: 2 pole terminal clamp

	Measuring range in ppm	Resolution in ppm	Output Output resistance	Nominal slope (at pH 7.2) in mA/ppm	Voltage supply	Galvanic isolation required in the measuring device/controller *	Connection
CL4.2MA0.5	0.005...0.500	0.001	4...20 mA uncalibrated	32.0	12...30 VDC R _L 50Ω...R _L 900Ω	yes	2-pole terminal (2 x 1 mm ²) Recommended: Round cable ∅ 4 mm 2 x 0.34 mm ²
CL4.2MA2	0.005...2.000	0.001		8.0			
CL4.2MA5	0.05...5.00	0.01		3.2			
CL4.2MA10	0.05...10.00	0.01		1.6			
CL4.2MA20	0.05...20.00	0.01		0.8			
CL4.2MA-100	0.5...100.0	0.1		0.16			
CL4.2MA-200	0.5...200.0	0.1		0.8			

* for further information see brochure 'Technical information // galvanic isolation' (in the download area of our website www.reiss-gmbh.com)

(Subject to technical changes!)

4.2 Electrical connection: 5 pole M12 plug-on flange

	Measuring range in ppm	Resolution in ppm	Output Output resistance	Nominal slope (at pH 7.2) in mA/ppm	Voltage supply	Galvanic isolation required in the measuring device/controller *	Connection
CL4.2MA0.5-M12	0.005...0.500	0.001	4...20 mA uncalibrated	32.0	12...30 VDC R _L 50Ω...R _L 900Ω	yes	5-pole M12 plug-on flange Function of wires: PIN1: n. c. PIN2: +U PIN3: -U PIN4: n c. PIN5: n. c.
CL4.2MA2-M12	0.005...2.000	0.001		8.0			
CL4.2MA5-M12	0.05...5.00	0.01		3.2			
CL4.2MA10-M12	0.05...10.00	0.01		1.6			
CL4.2MA20-M12	0.05...20.00	0.01		0.8			
CL4.2MA-100-M12	0.5...100.0	0.1		0.16			
CL4.2MA-200-M12	0.5...200.0	0.1		0.8			

* for further information see brochure 'Technical information // galvanic isolation' (in the download area of our website www.reiss-gmbh.com)


(Subject to technical changes!)

Spare Parts


Type	Membrane cap	Electrolyte	Emery	O-ring
For all CL4.2	M20.2 Art. no. 11011.1	ECL1, 100 ml Art. no. 11001	S1 Art. no. 11908	14 x 1.8 NBR Art. No. 11806

(Subject to technical changes!)

Slope of TARAbase CL4 versus pH

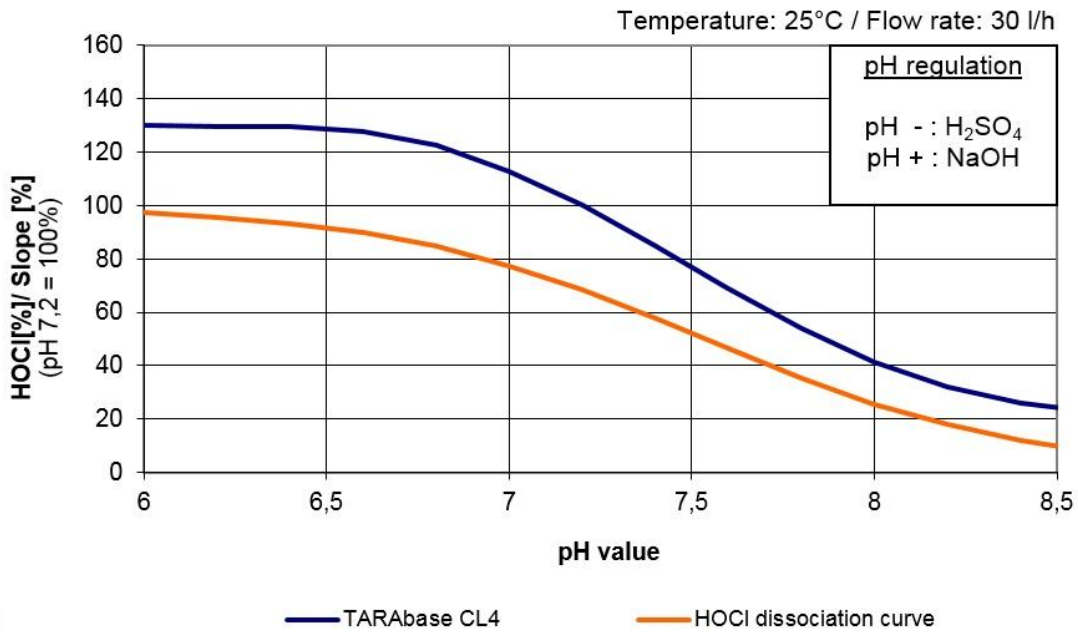

Slope of TARAbase CL4 versus Flow rate

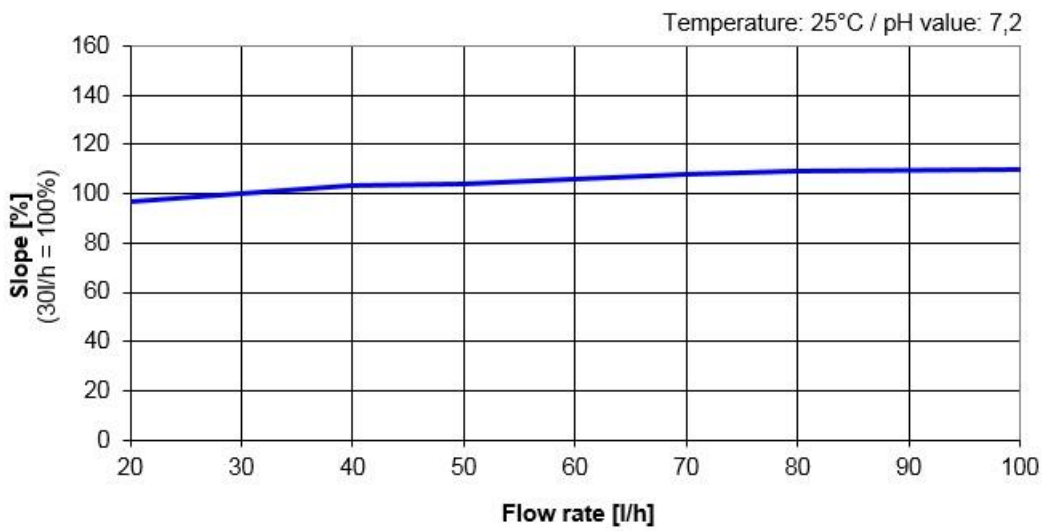

This values are only valid for the probe housing FLC1 / FLC3

CL4 Discharge